

Instructions For Use





EZ Reach™ Sponge Sampling Device


Watch Demonstration Video

US Patent 8,127,627B2


<https://www.worldbioproducts.com/ezreach-sponges.html>

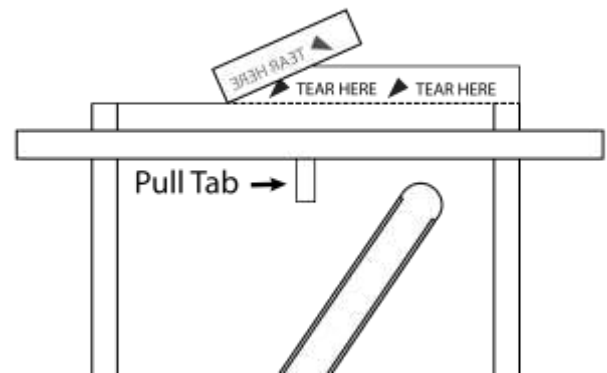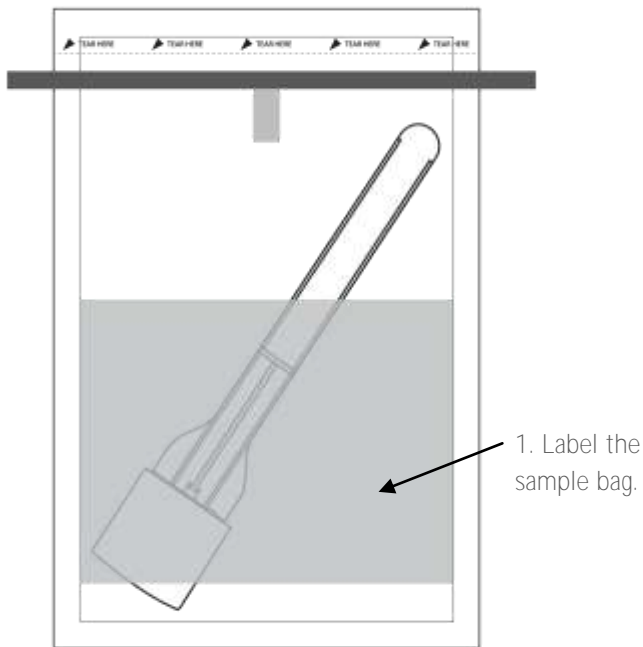


2. Tear off the top of the bag where indicated. Pull tabs to open bag. If needed, add a collection solution to hydrate the dry sponge device.

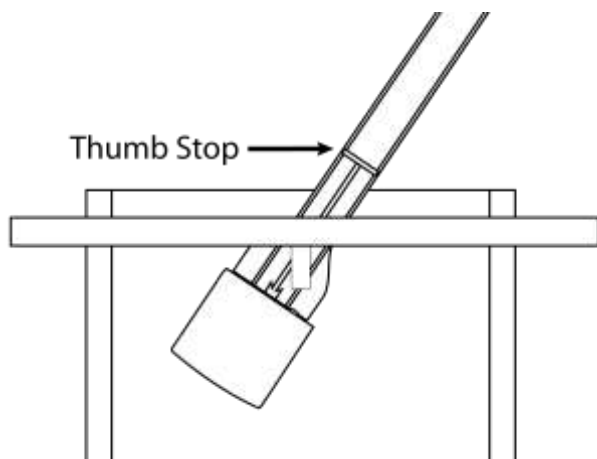


3. Keeping hands outside the bag, guide the handle out the top of the bag. Grasp the handle above the thumb stop and remove the device.

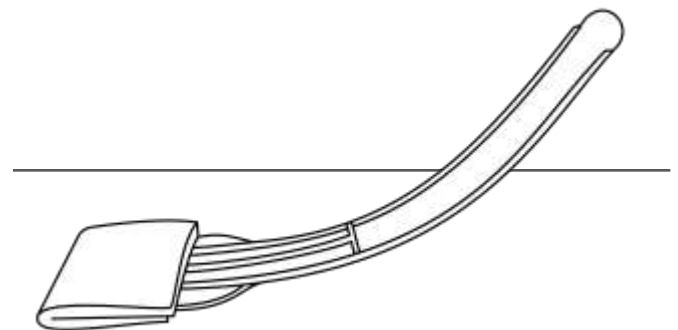


4. Press down firmly and flex the handle to ensure the entire sponge head makes full contact with the sample surface.

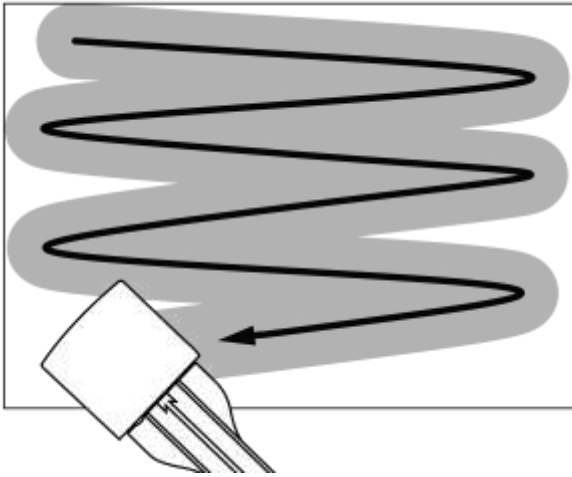


5. Vigorously scrub back and forth in one direction across the sample surface.

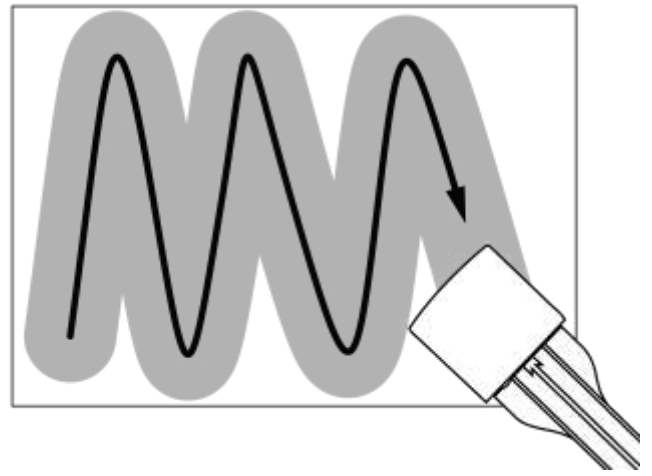

6. FLIP the sampling device over. Change direction 90° and vigorously scrub back and forth across the same surface area.

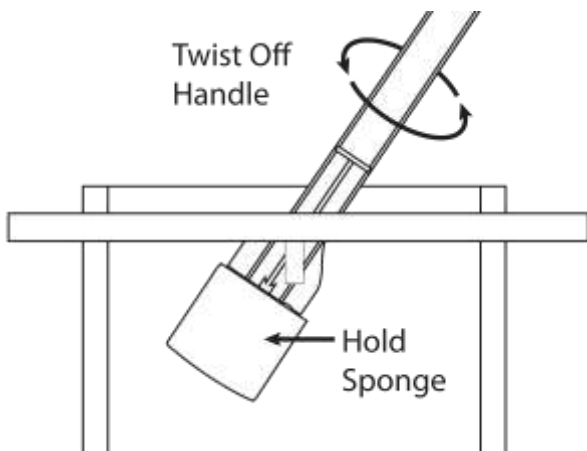

7. Return sampling device to the bag. Do not insert past the thumb stop. Hold sponge from the outside of the bag and twist off the handle by turning counter-clockwise.

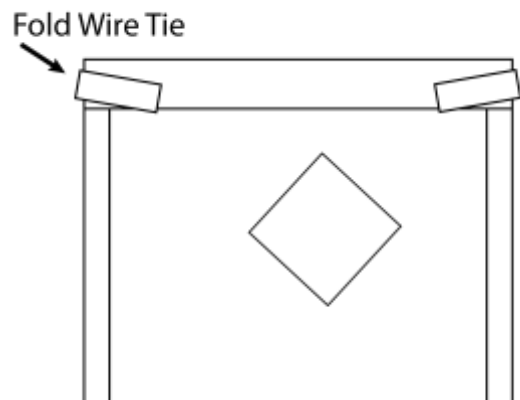

8. Roll down the top of the sample bag several times and fold wire ties over to securely close. Send to a laboratory for analysis.

Limitation of Liability:

World Bioproducts LLC shall not be liable for any special or consequential damages that result from the use of, or the inability to use, these materials or the performance of the products, even if World Bioproducts LLC has been advised of the possibility of such damages. Applicable law may not allow the limitation of exclusion of liability or incidental or consequential damages, so the above limitation or exclusion may not apply to you.

For In-Vitro Use Only

Safety Data Sheets & Certificates of Analysis available upon request.
Refer to package label for storage information.

World Bioproducts, LLC
Call 877-260-6441 / Mail PO Box 947, Bothell, WA 98041
Email orders@worldbioproducts.net / Visit worldbioproducts.com



Instructions For Use




EZ Reach™ Sponge Sampling Device with GLOVES


US Patent 8,127,627B2

Watch Demonstration Video


<https://www.worldbioproducts.com/ezreach-sponges.html>

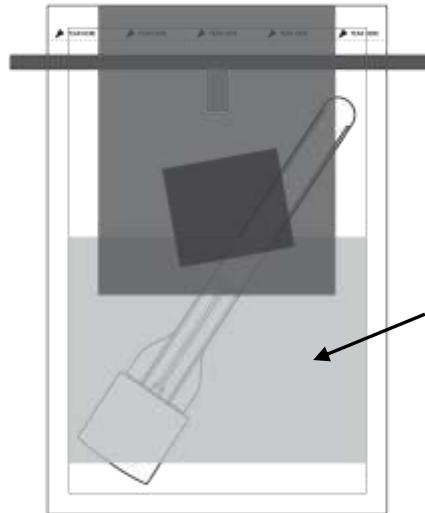


1. Write sample information onto sample bag.

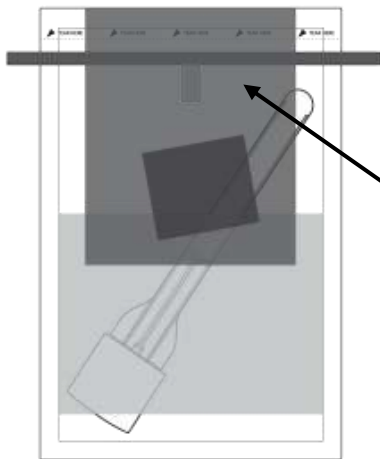


2. Tear off glove packet and put on gloves.

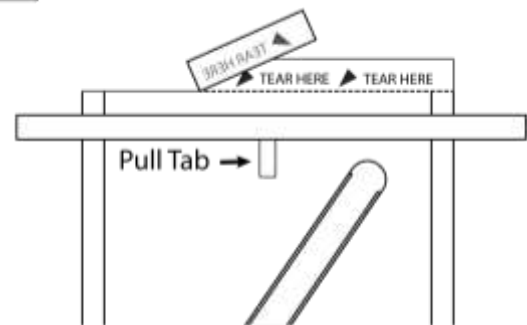


3. Tear off the top of the bag where indicated. Pull tabs to open bag. If needed, add a collection solution to hydrate the dry sponge device.

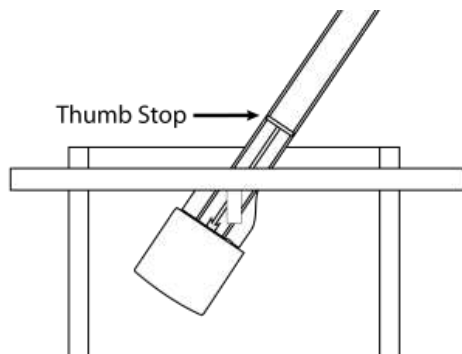


4. Keeping hands outside the bag, guide the handle out the top of the bag. Grasp the handle above the thumb stop and remove the device.

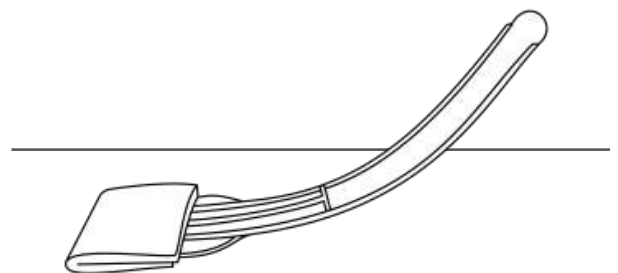


5. Press down firmly and flex the handle to ensure the entire sponge paddle makes full contact with the sample surface.

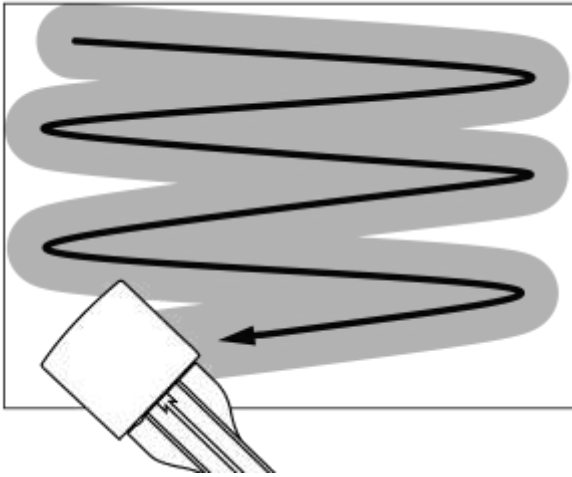


6. Vigorously scrub back and forth in one direction across the sample surface.

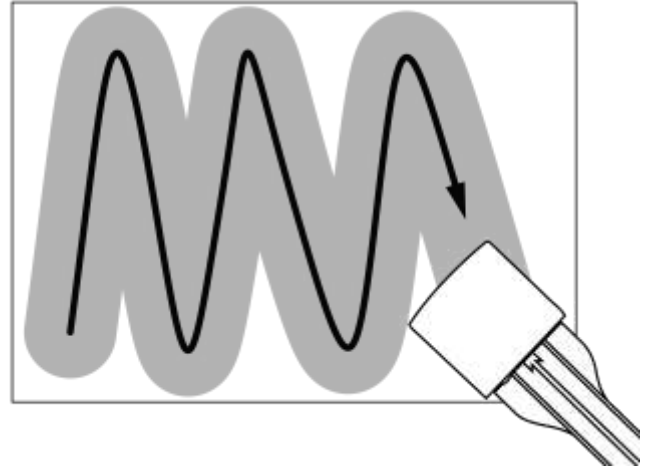

7. FLIP the sampling device over. Change direction 90° and vigorously scrub back and forth across the same surface area.

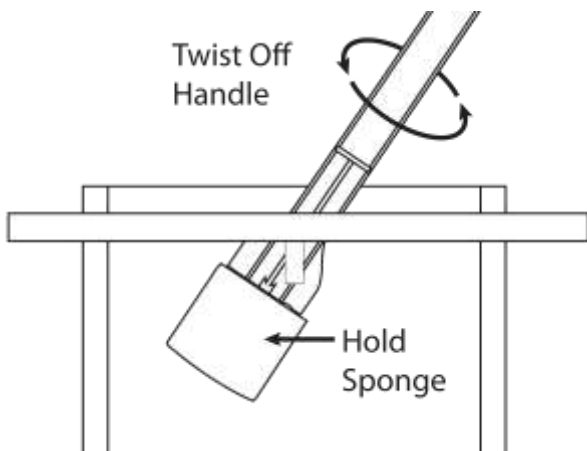

8. Return sampling device to the bag. Do not insert past the thumb stop. Hold sponge from the outside of the bag and twist off the handle by turning counter-clockwise.

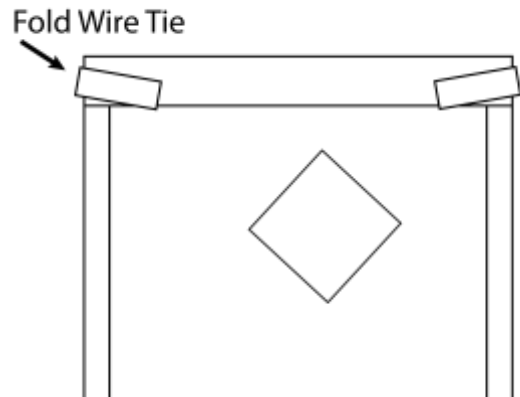

9. Roll down the top of the sample bag several times and fold wire ties over to securely close. Send to a laboratory for analysis.

Limitation of Liability:

World Bioproducts LLC shall not be liable for any special or consequential damages that result from the use of, or the inability to use, these materials or the performance of the products, even if World Bioproducts LLC has been advised of the possibility of such damages. Applicable law may not allow the limitation of exclusion of liability or incidental or consequential damages, so the above limitation or exclusion may not apply to you.

For In-Vitro Use Only

Safety Data Sheets & Certificates of Analysis available upon request.
Refer to package label for storage information.

World Bioproducts, LLC
Call 877-260-6441 / Mail PO Box 947, Bothell, WA 98041
Email orders@worldbioproducts.net / Visit worldbioproducts.com

